


Calibrant Report - CR6+ -

Appendix B

Calib Lot #:1
Plan #: 20110822003

Spiked 0.005 mg/L, 0.05 mg/L and 0.25 mg/L in River Water

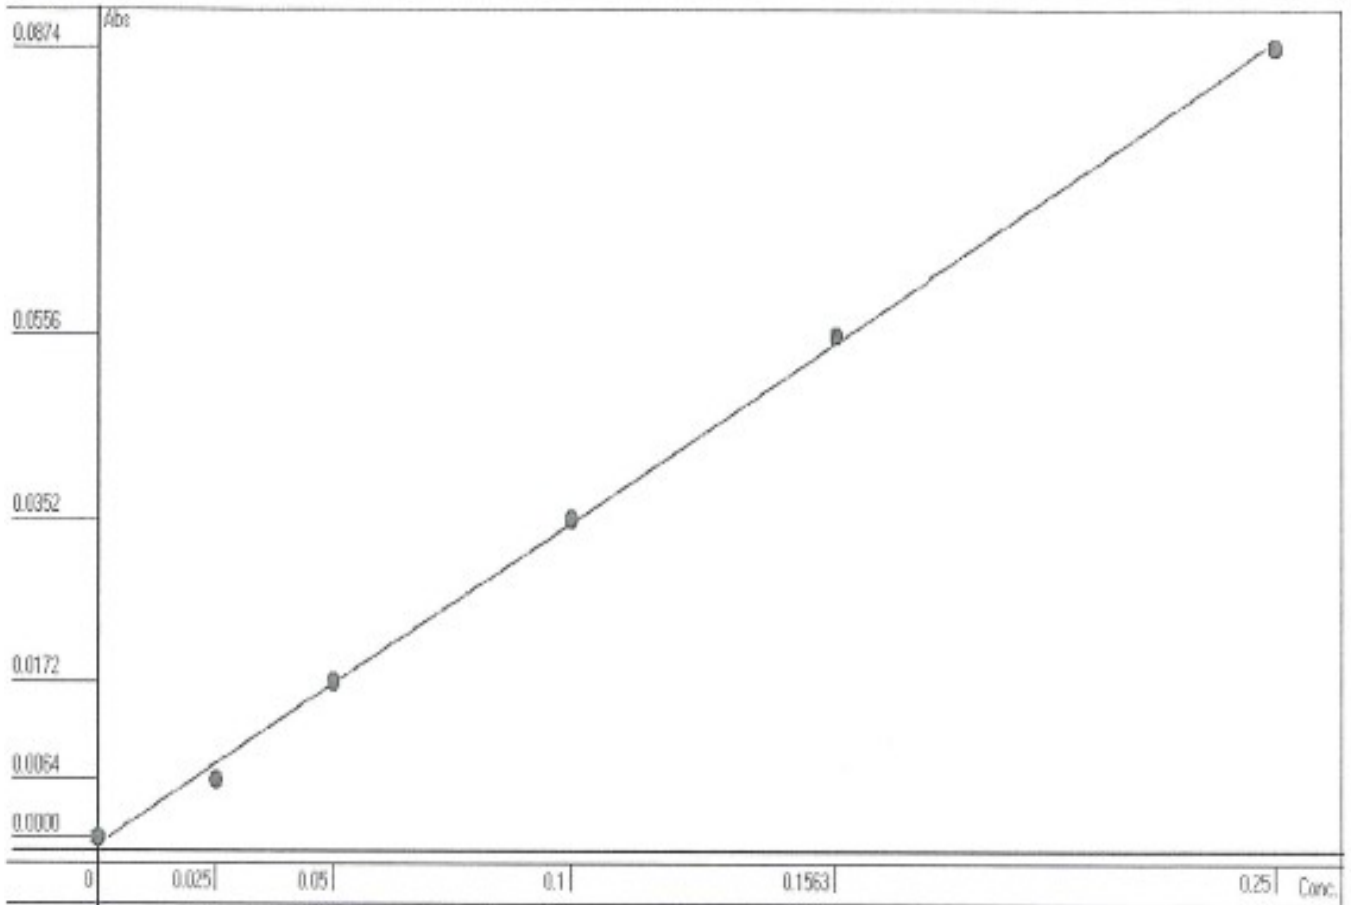

Point	OD	Conc.	Recalc Conc	% Error
1	0.0000	0	0.0022	0.22
2	0.0064	0.025	0.0202	-19.20
3	0.0172	0.05	0.0506	1.20
4	0.0352	0.1	0.1012	1.20
5	0.0556	0.1563	0.1587	1.54
6	0.0874	0.25	0.2481	-0.76

Conc.= +2.8139*Abso +0.0022 R²=0.9991

RBL
0.0021
0